


Aroclor PCBs in Oil

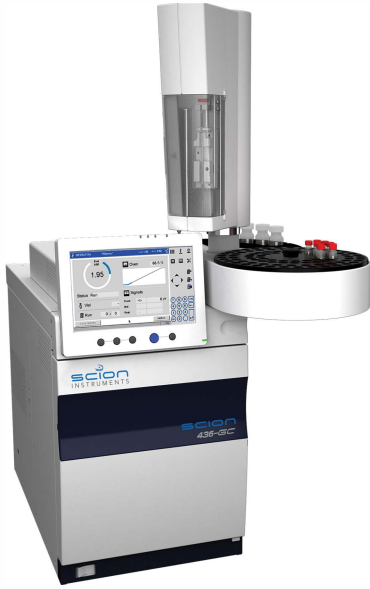


Hydrogen carrier, capillary column, ECD

Automated Aroclor identification (1242, 1254, 1260)

Automated Aroclor QTY correction for mixtures

0.5-50 ppm Calibration range in Oil

Fast Analysis time <8 mins

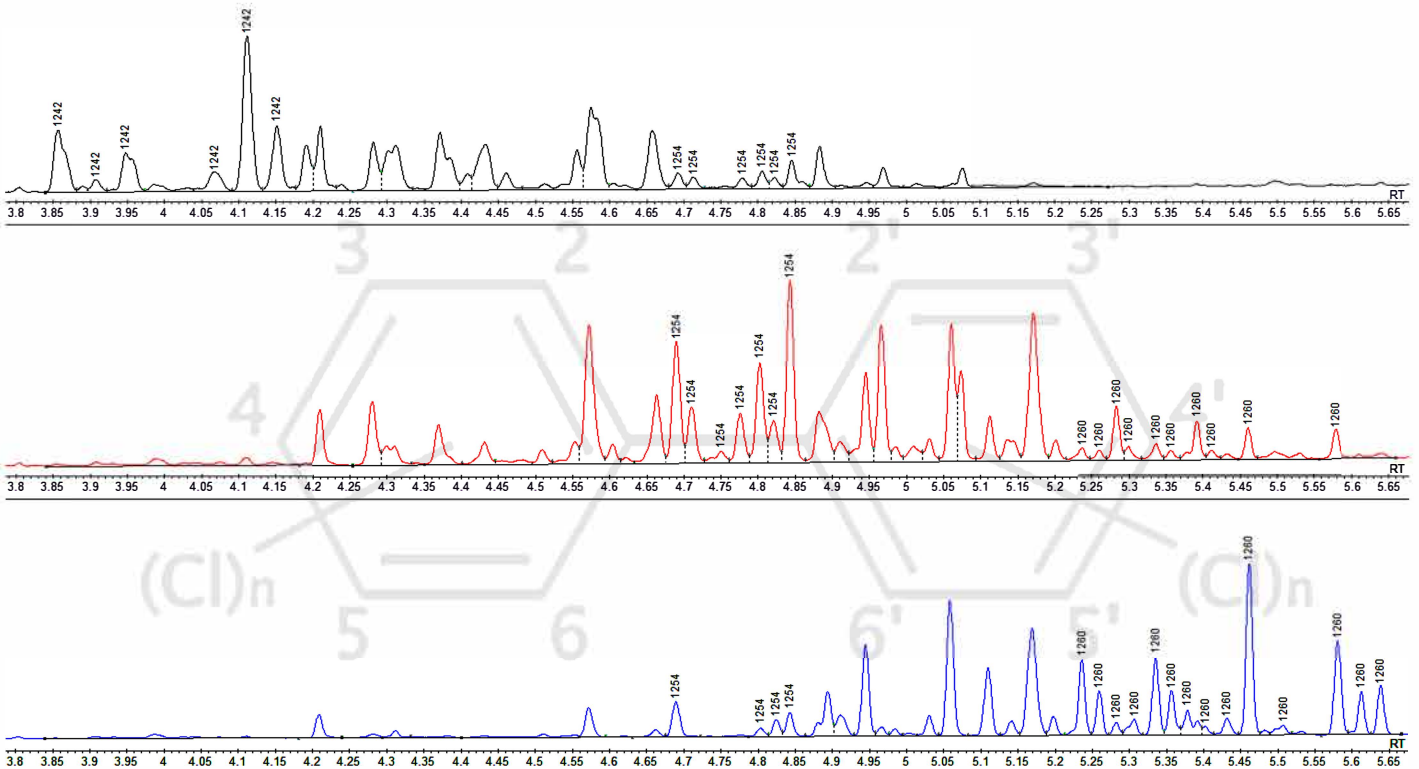

Analytical Solutions for Power Generation